

# *Certificate of Calibration*

Certificate Number: 32369

Document Number: 13265

***Customer Details:***

Customer Name: URS HOLDINGS INC

***Instrument Details:***

Manufacturer:	EXTECH INSTRUMENTS	Calibration Date:	January 15, 2010
Description:	NOISE DOSIMETER	Calibration Due:	January 15, 2011
Model Number:	407355	Cal. Interval:	12 MONTHS
Serial Number:	G032176	As Received:	INTERMITTENT
Equip. ID Number:	N/A		

***Environmental Details:***

Temperature: 21 Deg. +/- 5 C

Relative Humidity: 40 % +/- 15 %

***Procedures Used:***

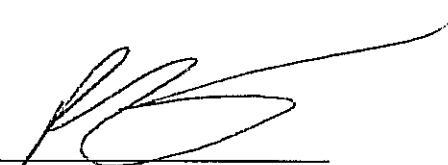
Calibration Procedure: 407355-C

## *Certification*

Extech Instruments certifies that the instrument listed above meets the specifications of the manufacturer at the completion of its calibration. Standards used are traceable to the National Institute of Standards and Technology (NIST), or have been derived from accepted values, natural physical constants, or through the use of the ratio method of self-calibration techniques. Methods used are in accordance with ISO 10012-1 and ANSI/NCSL Z540-1-1994. This certificate is not to be reproduced other than in full, except with prior written approval of Extech Instruments Corporation. All the calibration standards used have an accuracy ratio of 4:1 or better, unless otherwise stated.

Technicians Notes: Replaced Microphone.

Technician: ALAN WILSON

Approved By: 

# *Certificate of Calibration*

**Certificate Number: 37212**  
**Document Number: 16281**

*Customer Details:*

**Customer Name:** URS HOLDINGS INC

*Instrument Details:*

<b>Manufacturer:</b>	EXTECH INSTRUMENTS	<b>Calibration Date:</b>	May 5, 2010
<b>Description:</b>	SOUND LEVEL METER	<b>Calibration Due:</b>	May 5, 2011
<b>Model Number:</b>	407780	<b>Cal. Interval:</b>	12 MONTHS
<b>Serial Number:</b>	H008300	<b>As Received:</b>	OUT OF TOL
<b>Equip. ID Number:</b>	N/A		

*Environmental Details:*

**Temperature:** 21 Deg. +/- 5 C      **Relative Humidity:** 40 % +/- 15 %

*Procedures Used:*

**Calibration Procedure:** 407780-C

## *Certification*

Extech Instruments certifies that the instrument listed above meets the specifications of the manufacturer at the completion of its calibration. Standards used are traceable to the National Institute of Standards and Technology (NIST), or have been derived from accepted values, natural physical constants, or through the use of the ratio method of self-calibration techniques. Methods used are in accordance with ISO 10012-1 and ANSI/NCSL Z540-1-1994. This certificate is not to be reproduced other than in full, except with prior written approval of Extech Instruments Corporation. All the calibration standards used have an accuracy ratio of 4:1 or better, unless otherwise stated.

*Technicians Notes:*

**Technician:** TERI KING

**Approved By:** Teri King

# *Certificate of Calibration*

Certificate Number: 32314

Document Number: 2195

***Customer Details:***

Customer Name: URS HOLDINGS INC

***Instrument Details:***

Manufacturer:	EXTECH INSTRUMENTS	Calibration Date:	January 14, 2010
Description:	SOUND LEVEL CALIBRATOR	Calibration Due:	January 14, 2011
Model Number:	407766	Cal. Interval:	12 MONTHS
Serial Number:	Z088929	As Received:	IN TOLERANCE
Equip. ID Number:	N/A		

***Environmental Details:***

Temperature: 21 Deg. +/- 5 C

Relative Humidity: 40 % +/- 15 %

***Procedures Used:***

Calibration Procedure: EICM407766-CP

## *Certification*

Extech Instruments certifies that the instrument listed above meets the specifications of the manufacturer at the completion of its calibration. Standards used are traceable to the National Institute of Standards and Technology (NIST), or have been derived from accepted values, natural physical constants, or through the use of the ratio method of self-calibration techniques. Methods used are in accordance with ISO 10012-1 and ANSI/NCSL Z540-1-1994. This certificate is not to be reproduced other than in full, except with prior written approval of Extech Instruments Corporation. All the calibration standards used have an accuracy ratio of 4:1 or better, unless otherwise stated.

**Technicians Notes:**

Technician: ALAN WILSON

Approved By: 